


Installation plan

I-Track


- Suggested height of countertop: pharmacy countertop: approximately.: 40"
- Clearance in front of the device: minimum space for a counting tray
- Clearance on one side of the device: approximately 8 inches to accommodate a barcode scanner

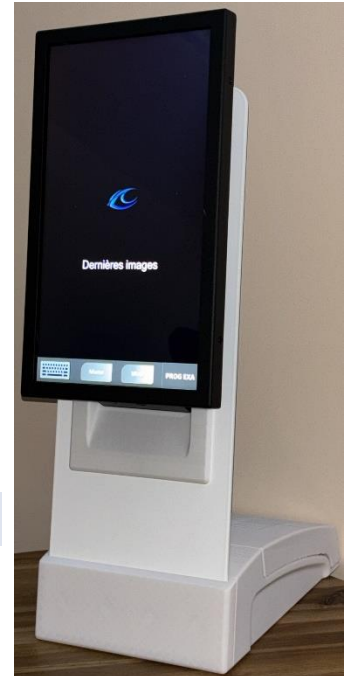

Items required near the device installation site

- One Electrical outlet
- One Network connection (DSL)

Device Dimension

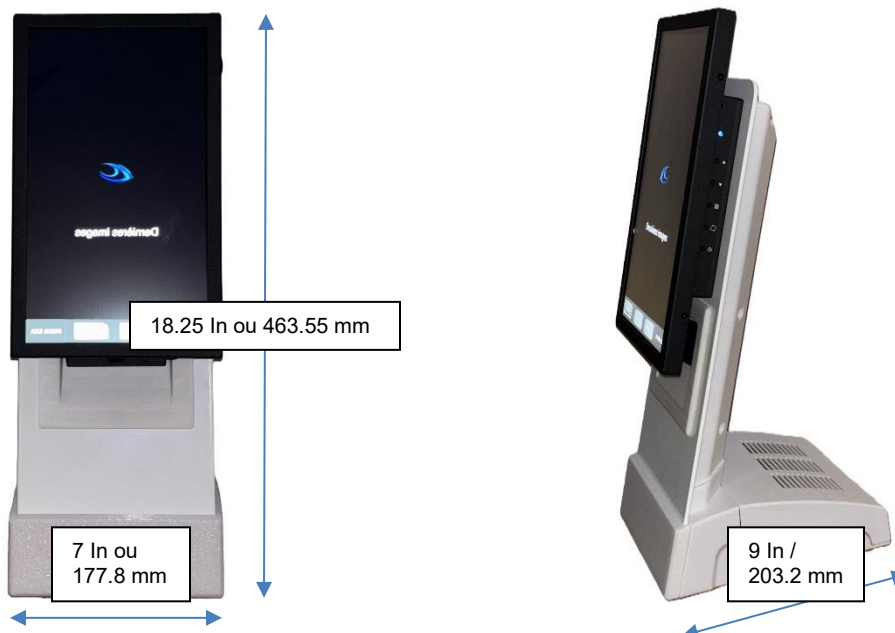

Date de révision : 20-02-2023